

Figure 1


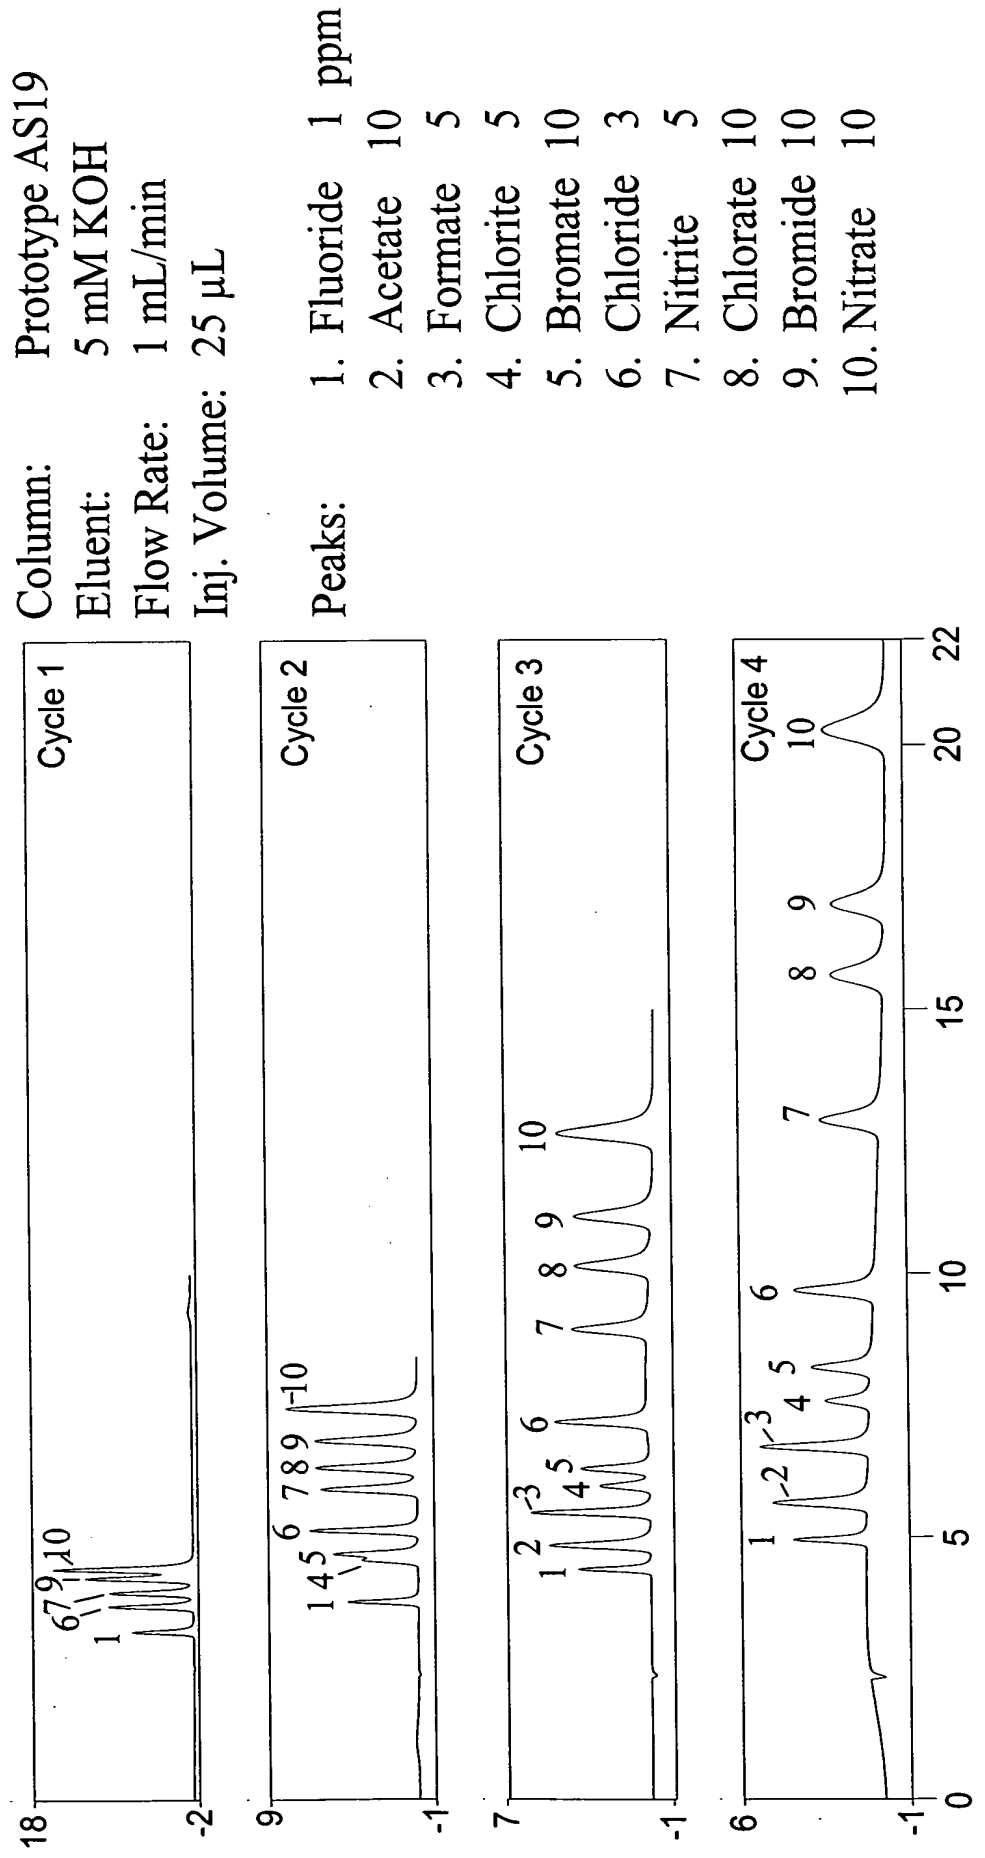


Figure 2

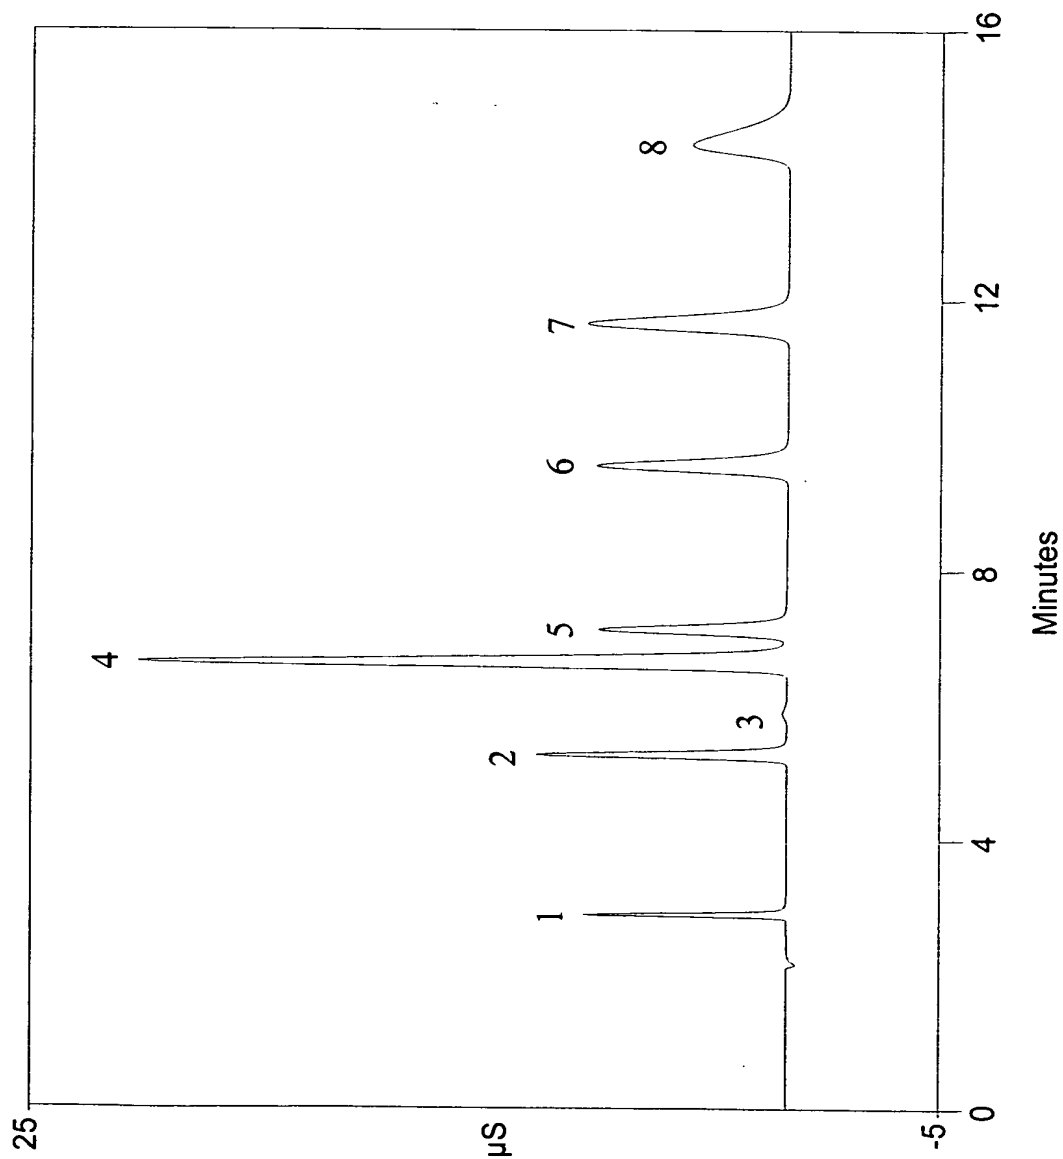

Column: Prototype AS19
Eluent: 35 mM KOH
Flow Rate: 1 mL/min
Inj. Volume: 25 µL

Peaks:

1. Fluoride	1 ppm
2. Chloride	3
3. Carbonate	?
4. Sulfate	15
5. Nitrite	5
6. Bromide	10
7. Nitrate	10
8. Phosphate	15

Figure 3


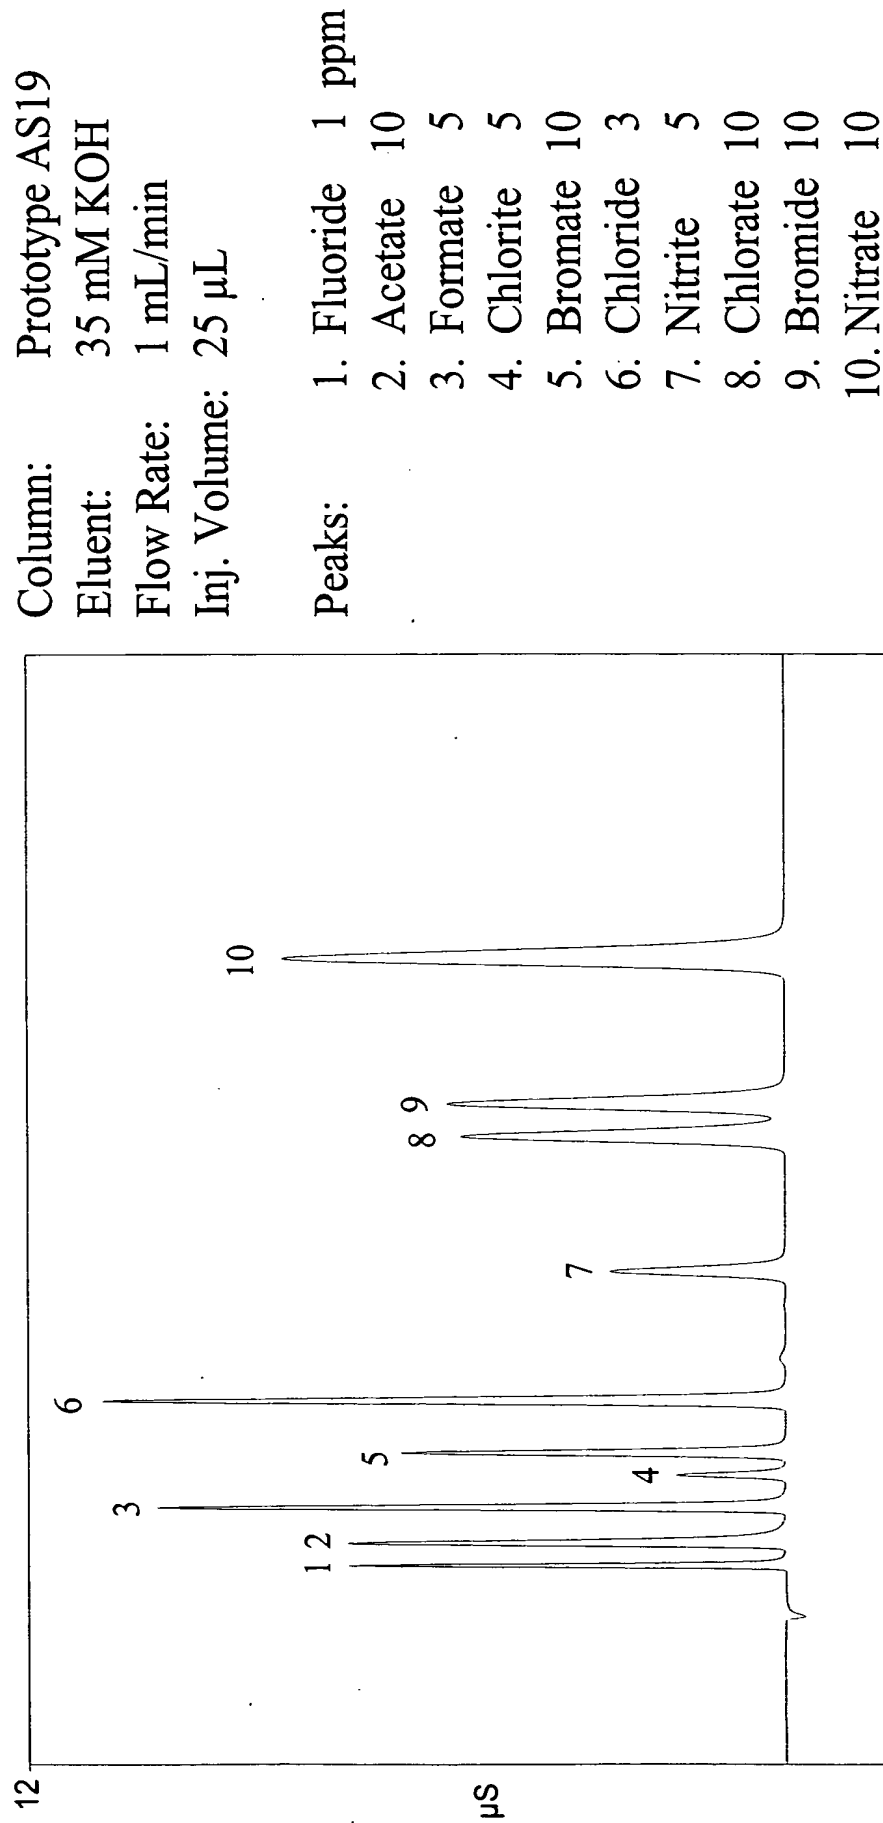


Figure 4

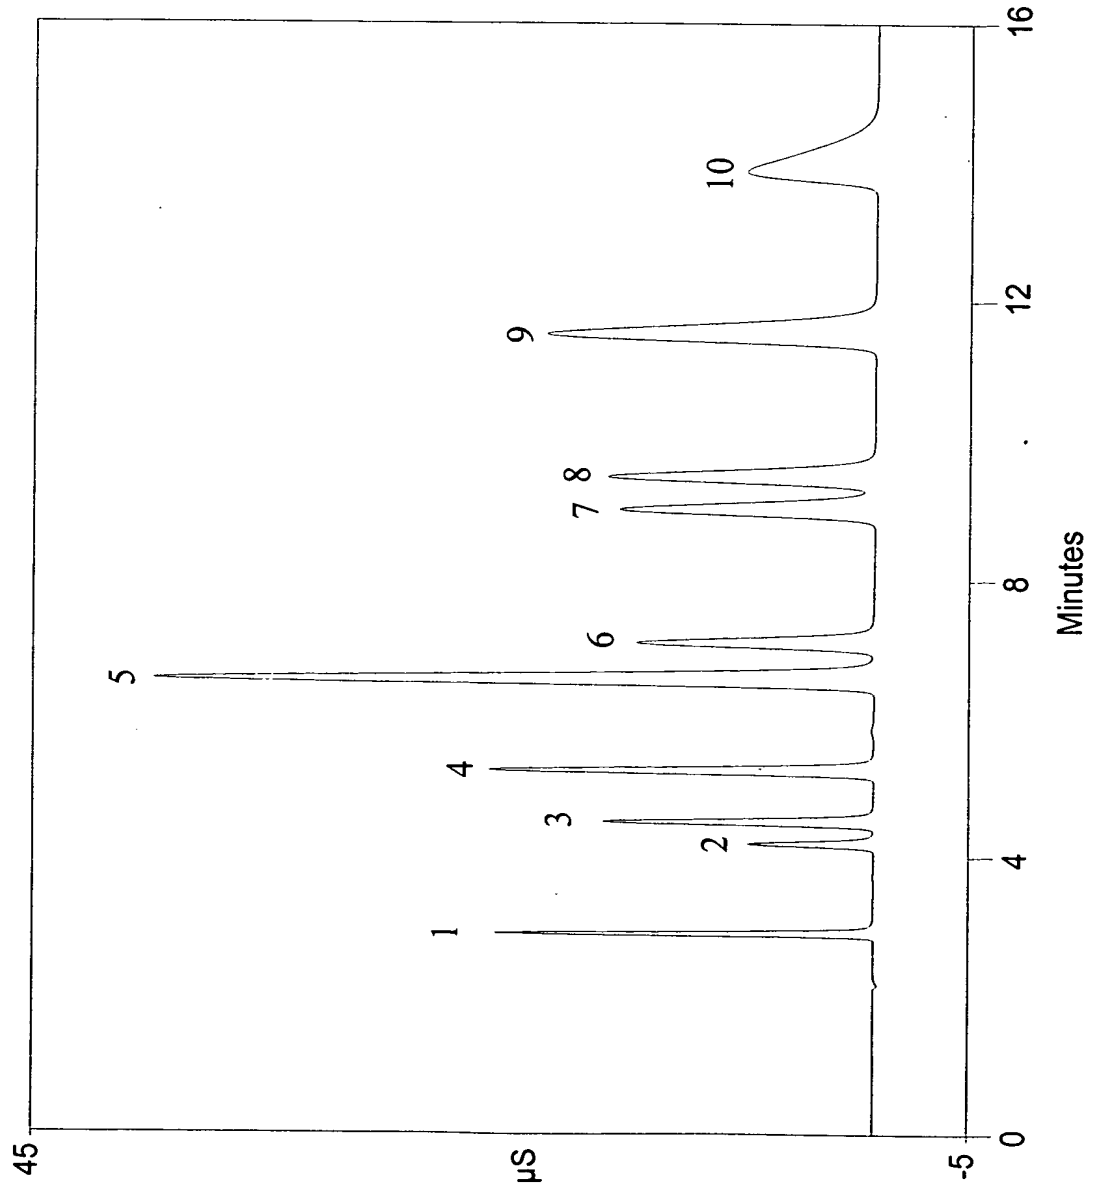

Column: Prototype AS19
 Eluent: 35 mM KOH
 Flow Rate: 1 mL/min
 Inj. Volume: 25 μL

Peaks:

1. Fluoride	3
2. Chlorite	10
3. Bromate	20
4. Chloride	6
5. Sulfate	30
6. Nitrite	15
7. Chlorate	25
8. Bromide	25
9. Nitrate	25
10. Phosphate	40

Figure 5

